

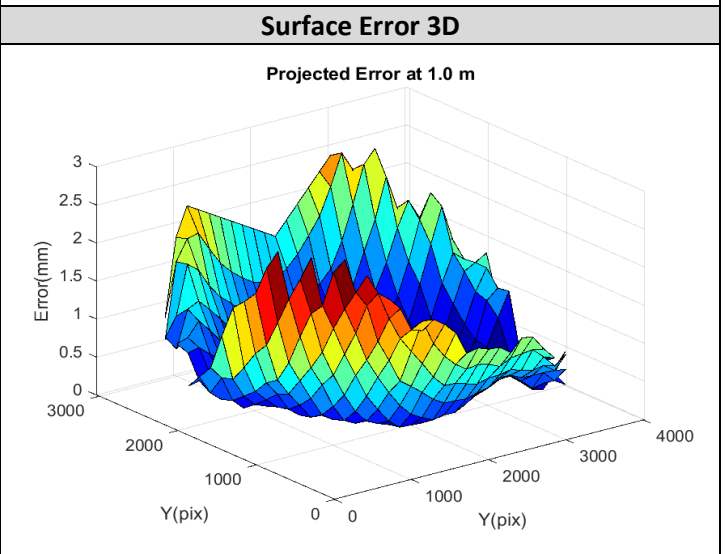
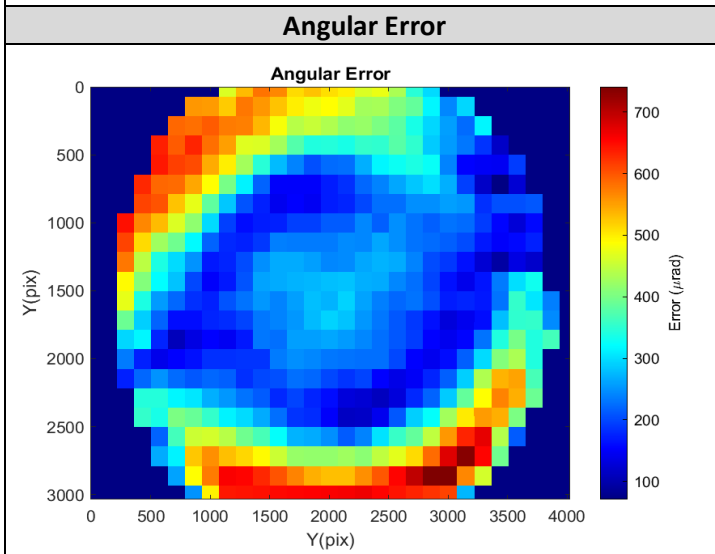


# Calibration ID: Sample EO89-340

Camera Information			Calibration Summary	
Part Information	Order Number		<b>Intrinsic Parameters</b> EFLx EFLy: [1631.1 1631.0] pixels PPx PPy: [2007.3 1579.3] pixels Radial Distortion Coeff: [0.0071 -0.0022 0.0032 -0.0007]	
	Order Date			
	Revision	A		
	Date Recorded	09-Apr-2024 19:20:50		
Sensor	Part Number	ACA4024-29um	<b>Extrinsic Parameters</b> Rx Ry Rz: [1.5722 0.0051 1.5630] rad Euler XYZ Intrinsic x y z: [0.01571 0.01321 -0.01183] m	
	Serial Number	24686169		
	Sensor Size	4024 x 3036		
Lens	Part Number	89340		
	Serial Number	0001		
Intrinsic Summary	Reprojection Error [pix]	0.4534		
	Model Type	KannalaModel		

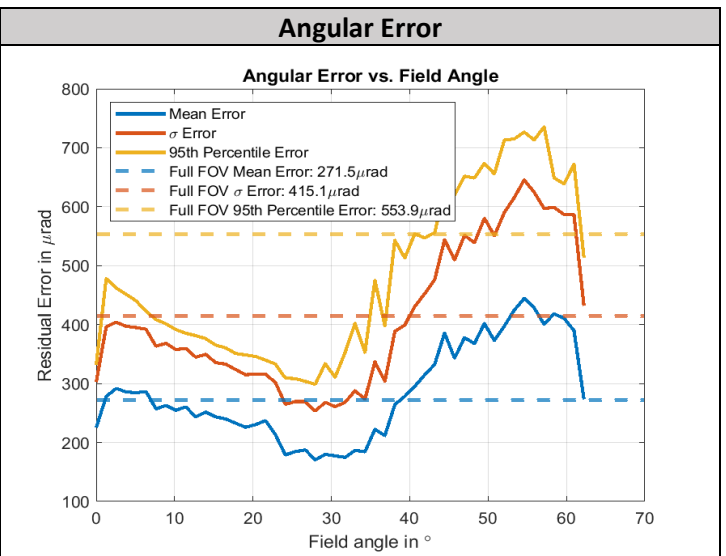

For more information on how to deploy this calibration, visit: [www.quartus.com/pixeltraq](http://www.quartus.com/pixeltraq) or scan

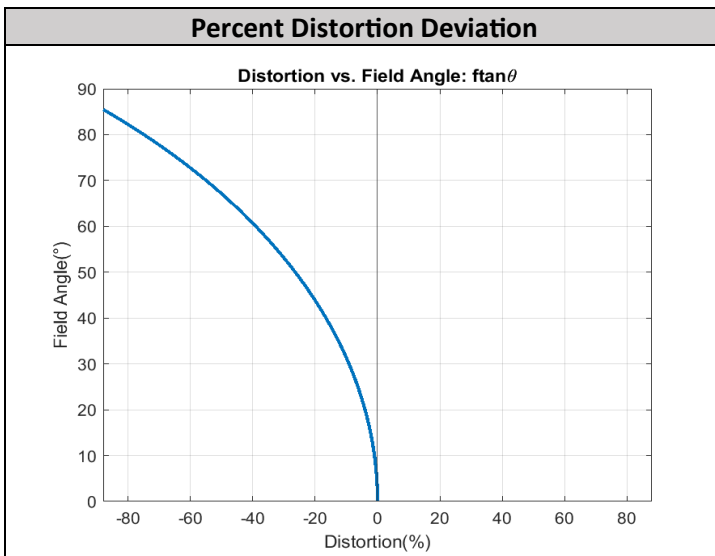