

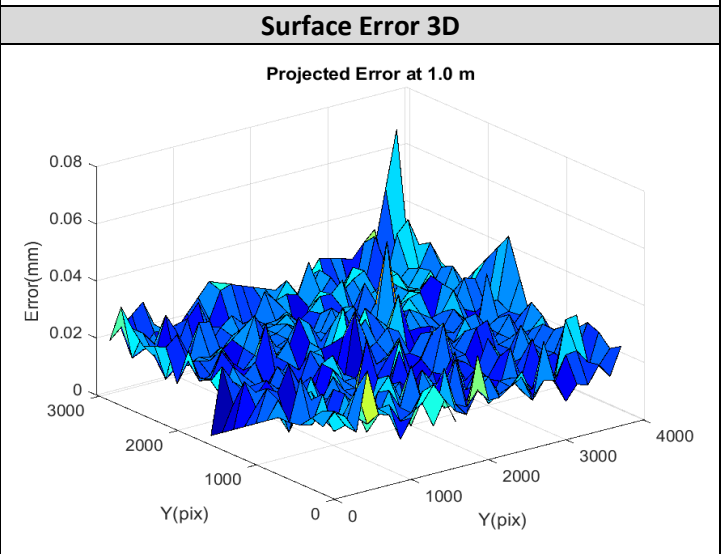
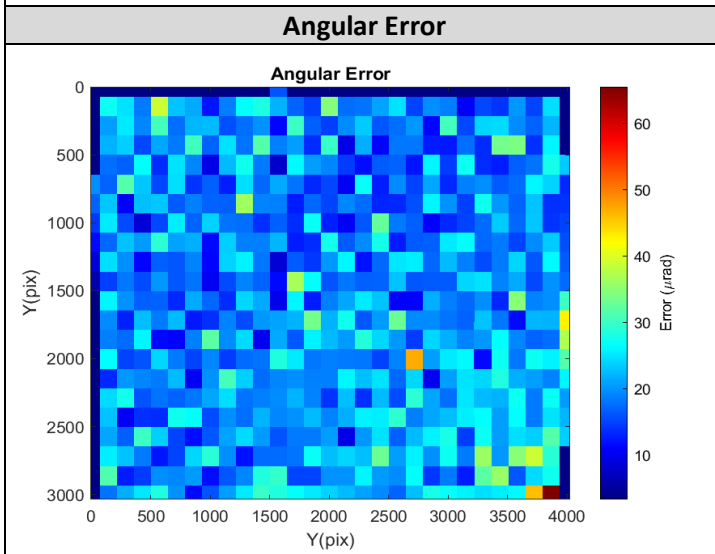


Calibration ID: Sample EO33-305

Camera Information			Calibration Summary	
Part Information	Order Number		Intrinsic Parameters EFLx EFLy: [13690.9 13690.8] pixels PPx PPy: [2035.3 1561.0] pixels Radial Distortion Coeff: [0.2489 -3.4291 140.2050 -1621.6856]	
	Order Date			
	Revision	A		
	Date Recorded	09-Apr-2024 18:58:39		
Sensor	Part Number	ACA4024-29um	Extrinsic Parameters Rx Ry Rz: [1.5681 0.0049 1.5742] rad Euler XYZ Intrinsic x y z: [0.01591 0.01411 -0.01905] m	
	Serial Number	24686169		
	Sensor Size	4024 x 3036		
Lens	Part Number	33305		
	Serial Number	0001		
Intrinsic Summary	Reprojection Error [pix]	0.2746		
	Model Type	KannalaModel		

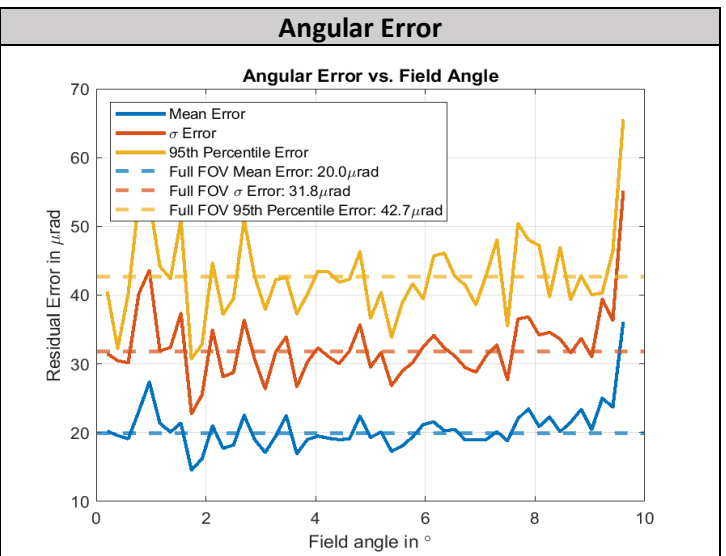

For more information on how to deploy this calibration, visit: www.quartus.com/pixeltraq or scan

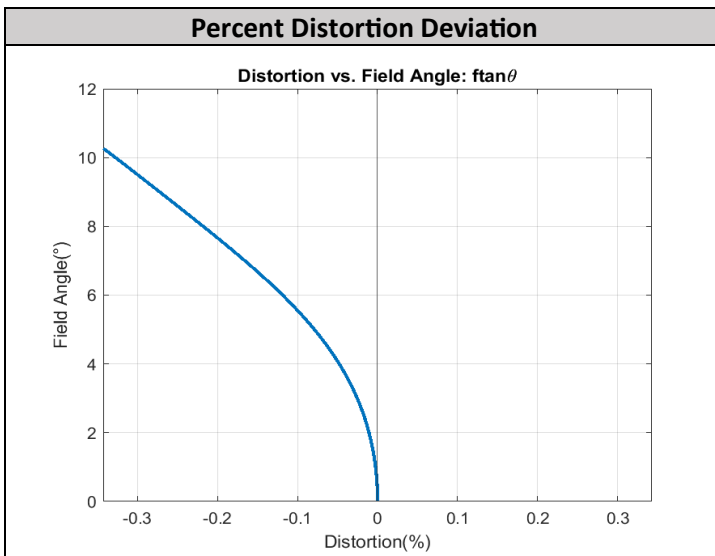