


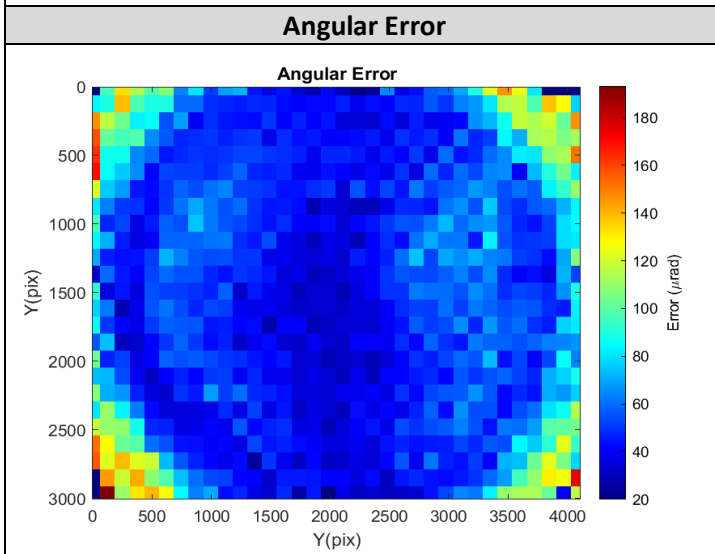


Calibration ID: Sample EO36-512

Camera Information			Calibration Summary	
Part Information	Order Number		Intrinsic Parameters EFLx EFLy: [4826.8 4827.5] pixels PPx PPy: [2021.5 1489.8] pixels Radial Distortion Coeff: [-0.1435 0.1001 -0.2275] Tangential Distortion Coeff: [-0.0007 0.0000] Tangential Distortion Poly Coeff: []	
	Order Date			
	Revision	A		
	Date Recorded	15-Mar-2024 15:58:58		
Sensor	Part Number	Genie Nano-M4020	Extrinsic Parameters Rx Ry Rz: [1.5699 -0.0018 1.5775] rad Euler XYZ Intrinsic x y z: [0.02137 0.01437 -0.03836] m	
	Serial Number	H2348628		
	Sensor Size	4112 x 3008		
Lens	Part Number	Edmund #36-512		
	Serial Number	N/A		
Intrinsic Summary	Reprojection Error [pix]	0.2870		
	Model Type	BrownConradyModel		

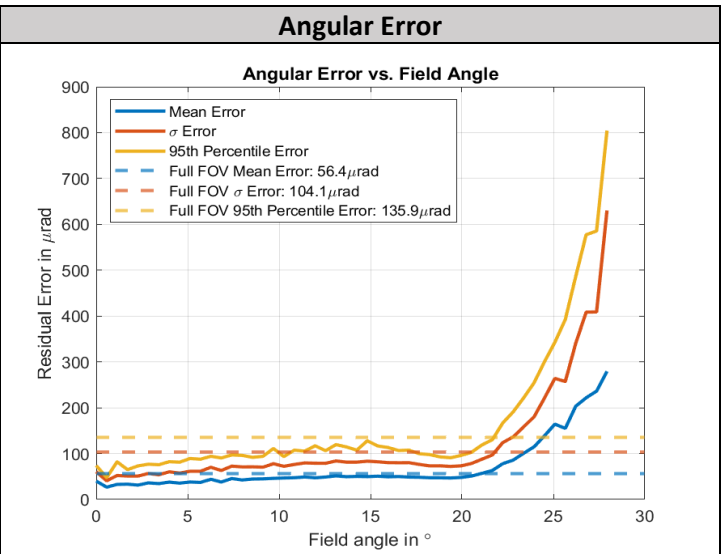

For more information on how to deploy this calibration, visit: www.quartus.com/pixeltraq or scan

